**Data Filename** TOX21\_201917\_TMS.D

Position 102 User Name Long Sample Name
Instrument Name


NCGC Tox21\_201917 from E06 SP109778


5975C\_MR

Acq Method C1

 $C1\_28\text{-}0\_2\_520\_mt384\_sndv.M$ 

### **User Chromatograms**

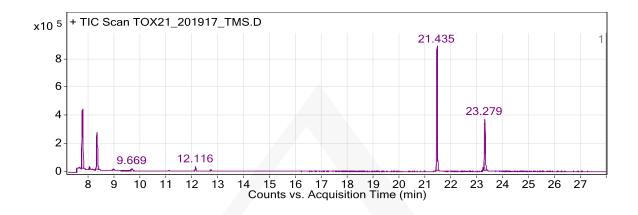


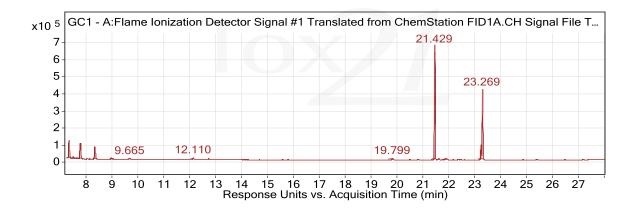

### **User Spectra**


#### **Spectrum Source**

Peak (1) in "+ TIC Scan"

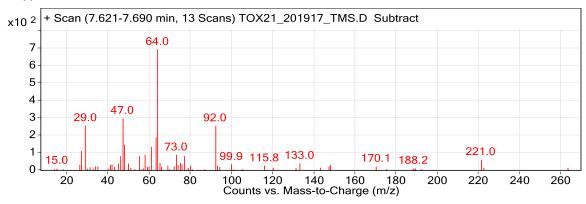


### **Spectrum Source**

Peak (2) in "+ TIC Scan"

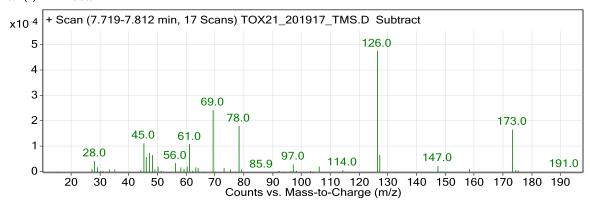

#### **Spectrum Source**


Peak (3) in "+ TIC Scan"

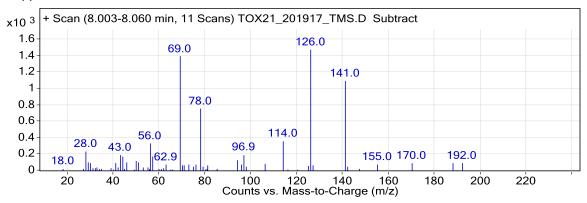

Page 2 of 5 Printed at: 10:23 AM on: 5/14/2014


#### **Spectrum Source**

Peak (4) in "+ TIC Scan"

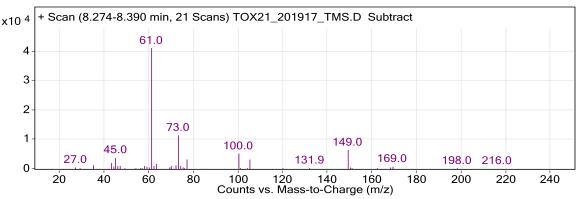


#### **Spectrum Source**

Peak (5) in "+ TIC Scan"

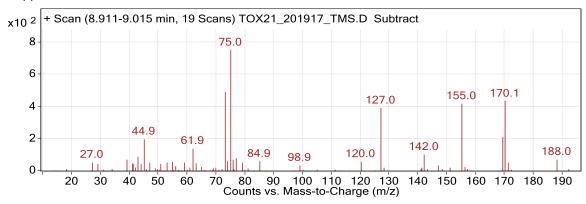

#### **Spectrum Source**


Peak (6) in "+ TIC Scan"

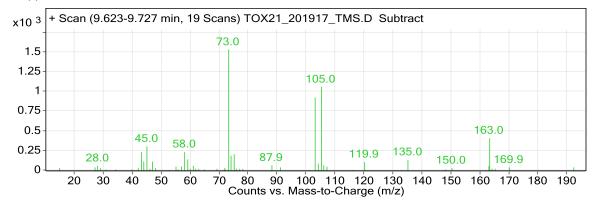




#### **Spectrum Source**

Peak (7) in "+ TIC Scan"

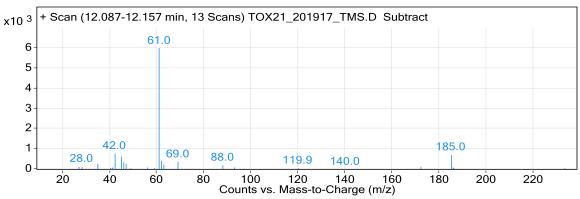


#### **Spectrum Source**

Peak (8) in "+ TIC Scan"

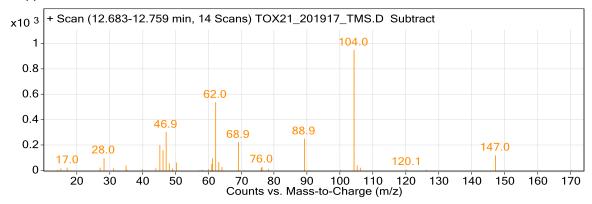

#### **Spectrum Source**


Peak (9) in "+ TIC Scan"

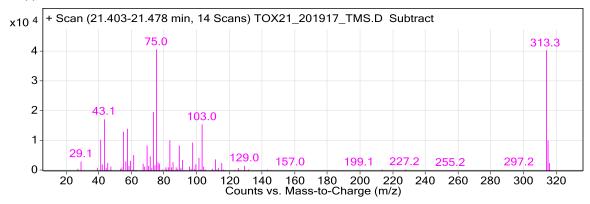

Agilent Technologies


#### **Spectrum Source**

Peak (10) in "+ TIC Scan"

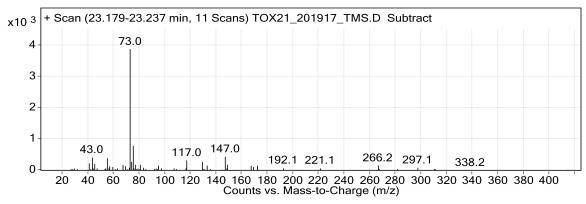

#### **Spectrum Source**

Peak (11) in "+ TIC Scan"

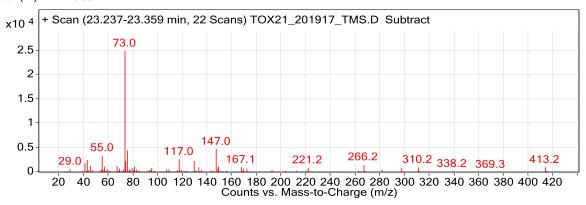

--- End Of Report ---

Printed at: 10:23 AM on: 5/14/2014